

APPLICATIONS OF CONDUCTING DIAMOND ELECTRODE FOR ELECTROANALYTICAL CHEMISTRY

Soo-Gil Park, Yasuaki Einaga*, Kensuke Honda*, Akira Fujishima**

Dept. of Industrial Chemical Eng., Chungbuk Nat'l Univ., Korea

*Dept. of Chemistry, Faculty of Science and Technology, Keio University, Japan

**Dept. of Applied Chemistry, School of Eng., The University of Tokyo, Japan

BDD has several superior electrochemical properties that are significantly different from those of other carbon allotropes, e.g., glassy carbon (GC), pyrolytic graphite (PG), and highly oriented pyrolytic graphite (HOPG), which have been widely used as electrode materials for many years. Diamond electrodes have recently been found to show high resistance to deactivation, via fouling, and insensitivity to dissolved oxygen. Here, Two kinds of experiments were carried out to show the excellent properties of BDD films as an electrode in electrochemical system.

Firstly, we generated ozone gas by BDD electrode in electrolysis method. Ozone generation concentration decreased c.a. 23% after 2000 hours' usage of PbO₂ electrode. On the other hand, it was almost constant even after 3000 hours' (more than 4 months) usage of diamond electrodes. However, in PbO₂ electrode system, the generated amount of ozone was gradually decreased resulted from structural degradation of electrode. This phenomenon was caused by application of high potential to the structurally weak electrode. These results show that diamond electrode is more stable for ozone generation by electrolysis method than PbO₂ electrode. Secondly, selective, stable determination of epinephrine (adrenalin) was achieved in cyclic voltammetric measurement carried out at electrochemically treated conductive boron-doped diamond electrode. Epinephrine, which is a component of neural transmission medium, takes effect on the transmission of nerve impulse. Many life phenomena are related to the concentration of epinephrine in blood. Previous techniques for the determination of epinephrine have been primarily based upon cation exchange, HPLC, CE, FIA, fluorimetry and sensors. However, the previous techniques suffered either tedious process or low sensitivity. In detecting epinephrine, a serious source of interference is the presence of electroactive constituent, including ascorbic acid at a typical concentration of 10⁻⁴M. In this work, we have found that it is possible to achieve selectivity for epinephrine in the presence of ascorbic acid solution after a simple electrochemical pretreatment of the diamond electrode.

BDD was used as an working electrode, Pt was used as the count electrode and A saturated calomel electrode (SCE) was used as the reference electrode. Electrochemical pretreatment was carried out by strong oxidation of BDD electrode. The voltammograms of epinephrine and AA before pretreat. the anodic peak(Ep,a) of epinephrine was +0.8±0.01V vs. SCE and Ep,a of ascorbic acid was 1.03±0.01V vs. SCE. These two peaks are overlapped after mixing of two chemicals owing to interference of AA. However, after simple pretreatment of BDD electrode, the peaks are separated originated epinephrine and AA respectively. These results were considered that oxidized diamond surface acquires surface dipoles as a result of introducing oxygen-containing functional groups, which then electrostatically

repel both anions and neutral molecules with strong dipoles; AA is negatively charged ion.

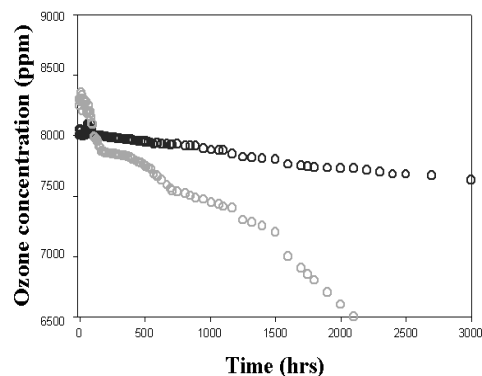


Fig. 1. Ozone generation Properties of diamond electrode and PbO₂ electrode (1M H₂SO₄, 2.3A/cm²)

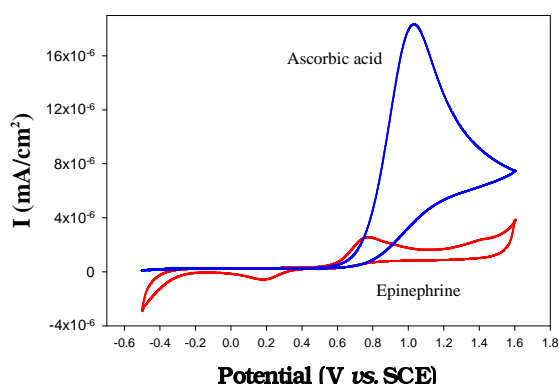


Fig. 2. Cyclic voltammograms for AA(1mM) and epinephrine

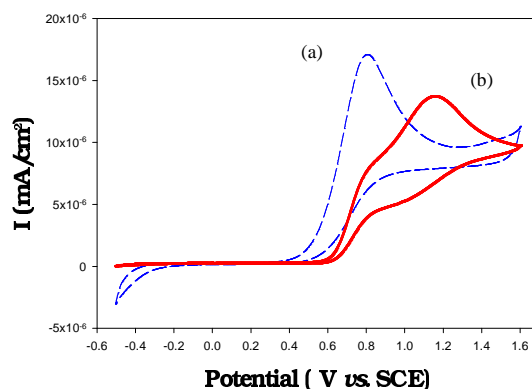


Fig. 3. Cyclic voltammograms for a 0.1M HClO₄ solution containing 0.1mM and 1mM ascorbic acid at untreated (a) and treated (b) diamond electrode.